

A.A. Jansson, Inc.

2070 Airport Rd
Waterford, MI 48327

Phone No. 248-674-4811 - Fax No. 248-674-1234

Certificate of Calibration

Web page: www.aajansson.com



Company: DIGIPAS TECHNOLOGIES INC.
Address: 200 SPECTRUM CENTER DRIVE
SUITE 300
IRVINE, CA 92618
Contact:
Job #: 59291-1

Doc #: 123501
Calibration Date: 3/12/2021
PO/Acct: DPO21-0006
Page: 1 of 3
Visual Condition: NEW GAGE
Date Received: 3/11/2021

Gage Desc: 2-AXIS ULTRA PRECISION LEVEL
Mfg: DIGIPAS TECHNOLOGIES
Procedure: AAJ CM-51.0

Cert #: DIG12A27115
Model#: DWL-9000 XY
Serial#: 12A27115


+ / - Tolerances: +1.200000 / -1.200000

Graph Scale: +0.100000

X AXIS-PLUS SLOPE

Nominal	Actual	Deviation
+0.000000	+0.000000	+0.000000
+825.000000	+824.800000	-0.200000
+1650.000	+1649.800	-0.200000
+2476.000	+2475.600	-0.400000
+3300.000	+3300.000	+0.000000
+4125.000	+4124.800	-0.200000
+4949.000	+4950.000	+1.000000
+6186.000	+6185.600	-0.400000

Measurement Uncertainty: ± 9 ARC SECONDS

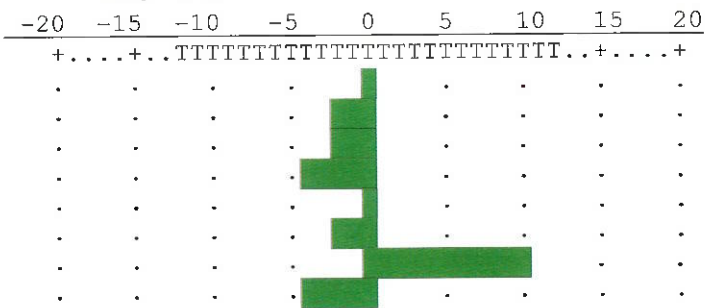


Graph Scale: +0.035000

X AXIS-MINUS SLOPE

Nominal	Actual	Deviation
+0.000000	+0.000000	+0.000000
+825.000000	+824.900000	-0.100000
+1650.000	+1649.900	-0.100000
+2476.000	+2475.800	-0.200000
+3300.000	+3299.900	-0.100000
+4125.000	+4124.900	-0.100000
+4949.000	+4949.600	+0.600000
+6186.000	+6185.500	-0.500000

Measurement Uncertainty: ± 9 ARC SECONDS

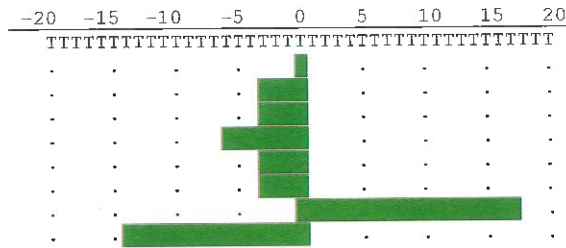


Graph Scale: +0.100000

DUAL AXIS-X PLUS SLOPE

Nominal	Actual	Deviation
+0.000000	+0.000000	+0.000000
+825.000000	+824.800000	-0.200000
+1650.000	+1649.800	-0.200000
+2476.000	+2475.600	-0.400000
+3300.000	+3299.200	-0.800000

Measurement Uncertainty: ± 9 ARC SECONDS

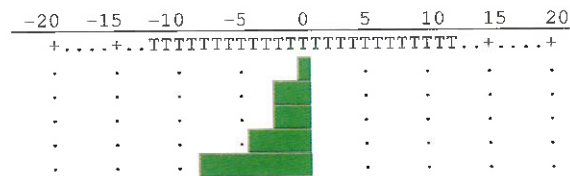


Graph Scale: +0.030000

DUAL AXIS-X MINUS SLOPE

Nominal	Actual	Deviation
+0.000000	+0.000000	+0.000000
+825.000000	+825.000000	+0.000000
+1650.000	+1650.000	+0.000000
+2476.000	+2475.700	-0.300000
+3300.000	+3299.500	-0.500000

Measurement Uncertainty: ± 9 ARC SECONDS

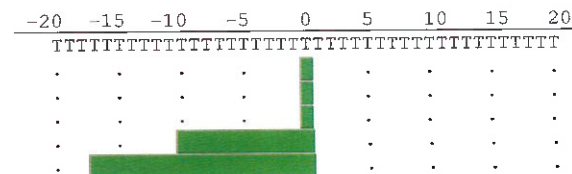

A.A. Jansson, Inc.

Certificate of Calibration

2070 Airport Rd
Waterford, MI 48327

Phone No. 248-674-4811 - Fax No. 248-674-1234

Web page: www.aaajansson.com

Page #: 2 of 3
Gage Desc: 2-AXIS ULTRA PRECISION LEVEL
Mfg: DIGIPAS TECHNOLOGIES
Procedure: AAJ CM-51.0


Doc #: 123501
Cert #: DIG12A27115
Model#: DWL-9000 XY
Serial#: 12A27115

DUAL AXIS-Y PLUS SLOPE

Nominal	Actual	Deviation
+0.000000	+0.000000	+0.000000
+825.000000	+825.000000	+0.000000
+1650.000	+1649.400	-0.600000
+2476.000	+2475.400	-0.600000
+3300.000	+3299.200	-0.800000

Measurement Uncertainty: ± 9 ARC SECONDS

Graph Scale: +0.100000

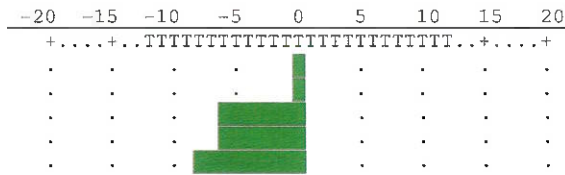


DUAL AXIS-Y MINUS SLOPE

Nominal	Actual	Deviation
+0.000000	+0.000000	+0.000000
+825.000000	+825.000000	+0.000000
+1650.000	+1650.500	+0.500000
+2476.000	+2475.800	-0.200000
+3300.000	+3299.500	-0.500000

Measurement Uncertainty: ± 9 ARC SECONDS

Graph Scale: +0.030000

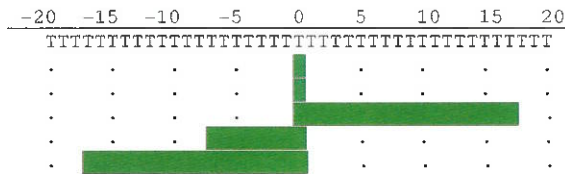

Comments:

CLEANED CALIBRATED AND CERTIFIED
DATA IS REPORTED IN ARC SECONDS
TEMPERATURE: 67.68° F

HUMIDITY: 35.9%

MANUFACTURER TOLERANCE:

± 0.2 ARC SECOND (0-100 ARC SECOND)

± 1.2 ARC SECONDS FOR OTHER ANGLES

We certify the equipment used for this calibration is traceable to NIST through one or more of the following numbers:

27124: 24" X 36" SURFACE PLATE

683/289434-17, 171871-U, L180827-4, L8580367368, RTRH16293094022118 Cal Date / Due Date: 8/13/2020 -- 8/13/2021

QC-SP: 5" SINE PLATE

16434265, 200048-U-1, L200819-6, L8581047797 Cal Date / Due Date: 12/21/2020 -- 12/21/2022

M-1: 97 Pcs Rect.

685-O-0000001278-20 Cal Date / Due Date: 3/8/2021 -- 3/8/2022

Gage Status: PASS

Unless otherwise noted in comments the following will apply;

1. Reported readings taken at 68°F ± 4° F Relative humidity less than 50%
2. Compliance statements will be binary and a simple acceptance decision rule will be applied, with no consideration for measurement uncertainty. The tolerance used will be per manufacturers Specification.
3. This is an endorsed Calibration Certificate (A2LA 1182.01) in accordance to ISO/IEC 17025:2017.
4. Data is "As-Found" and item is "Used."

Reported Measurement Uncertainties are based upon a 95% confidence level, k=2. This report shall not be reproduced, except in full, without written permission by A.A. Jansson, Inc. The results reported relate only to the items calibrated. Any number of factors may cause the subject of this calibration to drift out of calibration before the calibration interval has expired. Calibrations performed in accordance with the A.A. Jansson, Inc. Quality Assurance Manual Revision 10, Dated May 29, 2020. We certify the equipment used for this calibration is traceable to the International System of Units (SI) via standards traceable to NIST or other National Metrology Institutes (NMI).

